

Marquette University

e-Publications@Marquette

School of Dentistry Faculty Research and
Publications

Dentistry, School of

6-2017

A Method of Facilitating the Fabrication of Access Openings for Implant-Supported Complete Fixed Dental Prostheses

Seok-Hwan Cho
Marquette University

Geoffrey A. Thompson
Marquette University, geoffrey.thompson@marquette.edu

Follow this and additional works at: https://epublications.marquette.edu/dentistry_fac



Part of the [Dentistry Commons](#)

Recommended Citation

Cho, Seok-Hwan and Thompson, Geoffrey A., "A Method of Facilitating the Fabrication of Access Openings for Implant-Supported Complete Fixed Dental Prostheses" (2017). *School of Dentistry Faculty Research and Publications*. 311.

https://epublications.marquette.edu/dentistry_fac/311

Marquette University

e-Publications@Marquette

Dentistry Faculty Research and Publications/School of Dentistry

This paper is NOT THE PUBLISHED VERSION; but the author’s final, peer-reviewed manuscript. The published version may be accessed by following the link in the citation below.

The Journal of Prosthetic Dentistry, Vol. 117, No. 6 (June, 2017): 814-816. [DOI](#). This article is © Elsevier and permission has been granted for this version to appear in [e-Publications@Marquette](#). Elsevier does not grant permission for this article to be further copied/distributed or hosted elsewhere without the express permission from Elsevier.

Contents

Abstract.....	2
Technique.....	2
Discussion.....	5
Summary	5
References	6

A method of facilitating the fabrication of access openings for implant-supported complete fixed dental prostheses

Seok-Hwan Cho

Predocloral Prosthodontics and Biomaterials, Department of General Dental Sciences, Marquette University School of Dentistry, Milwaukee, WI

Geoffrey A. Thompson

Department of General Dental Sciences, Graduate Prosthodontics, Marquette University School of Dentistry, Milwaukee, WI

Abstract

This report describes a method for fabricating access openings for implant-supported complete fixed dental prostheses (ICFP) by using a dental milling machine and silicone putty matrix. The method can help clinicians achieve the accurate and precise fabrication of access openings for ICFPs without excessive grinding.

Implant-supported complete fixed dental prostheses (ICFPs) are successfully used to address problems found with complete removable dental prostheses such as instability and discomfort.^{1,2} However, one of the most common prosthetic complications has been the wear or fracture of acrylic resin teeth, requiring removal of the prosthesis for repair.^{3,4,5,6,7,8,9} Priest et al⁴ showed that fractured denture teeth or acrylic resin required repair 10 times in 5 patients. Purcell et al⁵ reported that tooth fracture and wear required tooth replacement 20 times in 13 patients and that prosthesis removal led to an excessively large access opening. Inaccurate access opening fabrication could create a loss of occlusal contacts because of unnecessary or excessive grinding.

This article describes the precise fabrication of access openings for ICFPs by using a dental milling machine (AF 30; Novvag AG) and a silicone putty matrix.

Technique

1. Adapt silicone (Aquasil EasyMix Putty Smart Wetting Impression Material; Dentsply Sirona) to the denture teeth after the tooth arrangement step and save the silicone matrix (Fig. 1).



Figure 1. Adapted silicone matrix on denture teeth after tooth arrangement.

2. Remove a denture tooth and insert a guide pin (Guide Pin Multi-unit 20 mm; Nobel Biocare) in order to visualize the direction of the implant placement (Fig. 2).

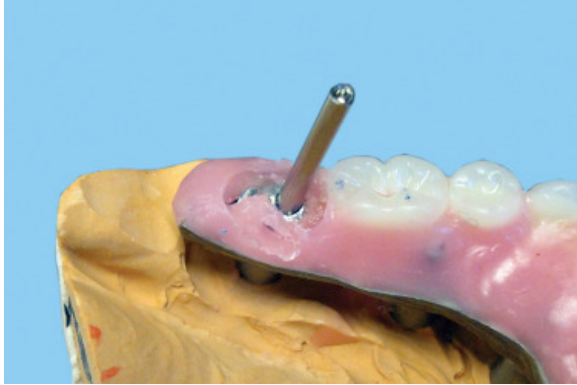


Figure 2. Guide pin inserted after removal of denture tooth.

3. Place the definitive cast on the table of a dental milling machine (AF 30; Nouvag AG) and insert a #6 round bur (H1.104.108; Komet USA) into the milling handpiece; then orient the table in order to make a guide pin parallel to the round bur (Fig. 3A). The round bur size is similar to the guide pin diameter (Fig. 3B).

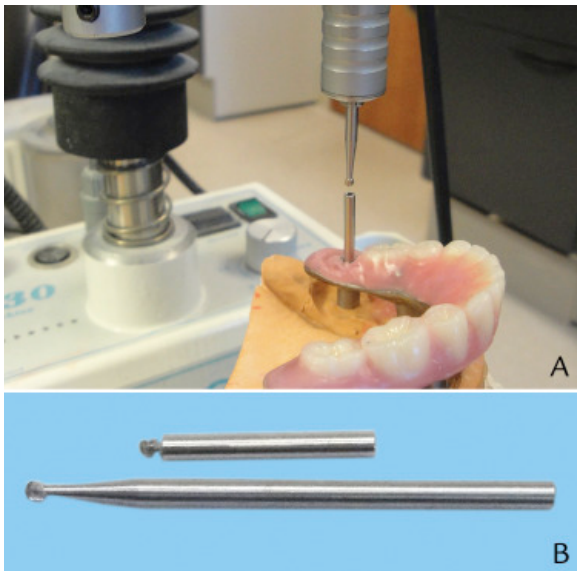


Figure 3. A, Orientation of table to make guide pin parallel to round bur direction. B, Similar size of round bur to guide pin diameter.

4. Without removing the definitive cast from the table, place the same denture tooth into the identical area by using the silicone matrix and stabilize the tooth with wax (Fig. 4A). The same bur direction is maintained during this procedure (Fig. 4B). Drill through the denture tooth to make an access opening (Fig. 4C).

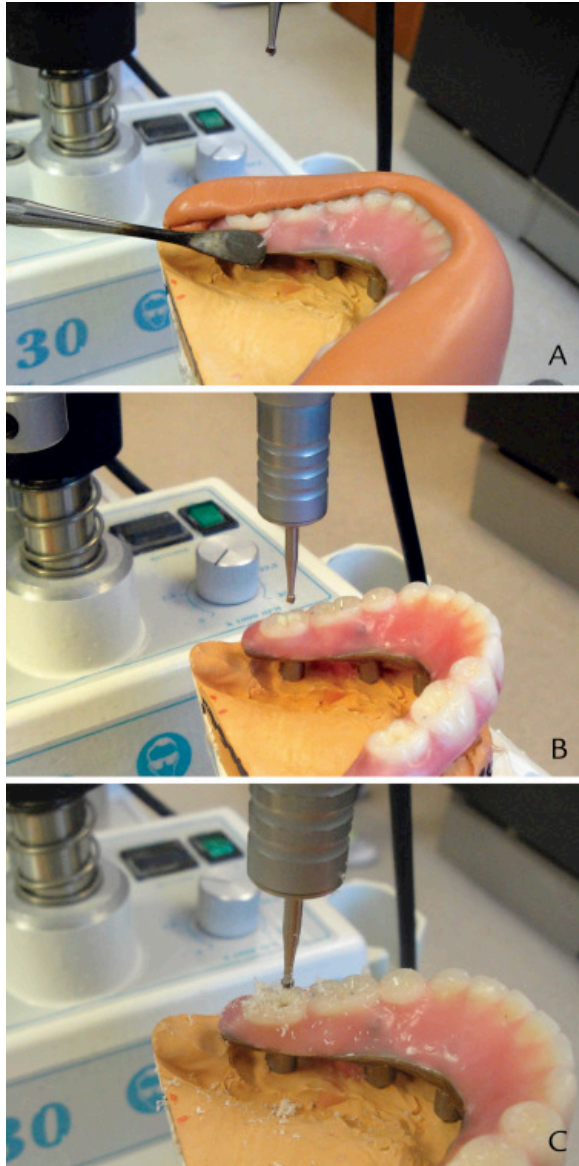


Figure 4. A, Same denture tooth placed into identical area with silicone matrix and wax. B, Maintained direction of bur after relocation of denture tooth. C, Drilling access opening through denture tooth.

5. Place a guide pin into the access opening through the denture tooth in order to verify the direction of the access opening (Fig. 5).

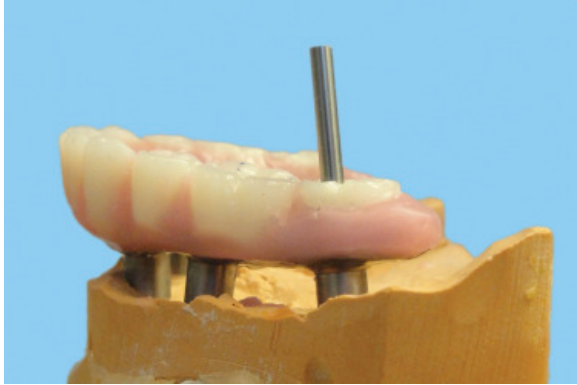


Figure 5. Verification with guide pin into access opening through denture tooth.

6. Repeat the other access openings using the same method. With this method, the precise opening through the denture teeth can be achieved without creating an excessively large opening (Fig. 6).

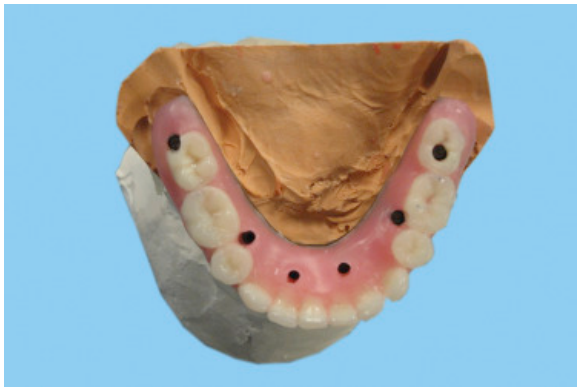


Figure 6. Access openings fabricated through denture teeth without excessive grinding.

Discussion

This article presents a method for fabricating accurate access openings for ICFPs, using a dental milling machine and silicone putty matrix.

The advantage of the method is the ability to reduce the grinding often observed with an arbitrary approach while producing an adequately sized access opening. Therefore, the method can reduce the potential fracture of the accessed denture teeth. One limitation of this technique is that the cast should be maintained in the exact same position during the whole procedure because the key to this method is the orientation of the attached bur and the cast. The cast should be secured on the milling table during grinding of the access hole. Another possible disadvantage of this technique would be the cost of the milling machine. However, this method will reduce the incidence of denture tooth fracture and chipping of ICFPs and expedite the access opening fabrication process.

Summary

A laboratory method of fabricating an accurate access opening for ICFPs by using both a dental milling machine and silicone putty matrix is described. The proposed technique not only improves the accuracy

and speed of making access openings but also reduces the chances of unnecessary or excessive grinding. This fabrication method will provide advantages to both clinicians and patients.

References

- 1 G.J. Christensen. **Treatment of the edentulous mandible.** J Am Dent Assoc, 132 (2001), pp. 231-233
- 2 G.A. Zarb. **Introduction to the Halifax Symposium: Toward optimized management of the edentulous predicament.** J Prosthet Dent, 79 (1998), pp. 3-4
- 3 T. Bozini, H. Petridis, K. Garefis, P. Garefis. **A meta-analysis of prosthodontic complication rates of implant-supported fixed dental prostheses in edentulous patients after an observation period of at least 5 years.** Int J Oral Maxillofac Implants, 26 (2011), pp. 304-318
- 4 G. Priest, J. Smith, M.G. Wilson. **Implant survival and prosthetic complications of mandibular metal-acrylic resin implant complete fixed dental prostheses.** J Prosthet Dent, 111 (2014), pp. 466-475
- 5 B.A. Purcell, E.A. McGlumphy, J.A. Holloway, F.M. Beck. **Prosthetic complications in mandibular metal-resin implant-fixed complete dental prostheses: a 5- to 9-year analysis.** Int J Oral Maxillofac Implants, 23 (2008), pp. 847-857
- 6 G.D. Quinn, A.A. Giuseppetti, K.H. Hoffman. **Chipping fracture resistance of denture tooth materials.** Dent Mater, 30 (2014), pp. 545-553
- 7 S.D. Heintze, D. Monreal, V. Rousson. **Fatigue resistance of denture teeth.** J Mech Behav Biomed Mater, 53 (2016), pp. 373-383
- 8 J. Ventura, E. Jiménez-Castellanos, J. Romero, F. Enrile. **Tooth fractures in fixed full-arch implant-supported acrylic resin prostheses: a retrospective clinical study.** Int J Prosthodont, 29 (2016), pp. 161-165
- 9 T. Sekinishi, S. Inukai, N. Murakami, N. Wakabayashi. **Influence of denture tooth thickness on fracture mode of thin acrylic resin bases: An experimental and finite element analysis.** J Prosthet Dent, 114 (2015), pp. 122-129